

Vitalograph®

2120 Storage Spirometer


Sample Printout from Inkjet Printer

ID: 040796-P1 Test Date: 04/07/1996 Time: 10:57:59
 Age: 45 Height: 182 cms Sex: M Ethnic Origin: Caucasian

Pre Test Quality Information Post Test Quality Information
 Variability - FVC: 0.7 FEV1: 0.6 Variability - FVC: 0.1 FEV1: 0.0
 Number of tests: 3 Number of tests: 3

ERS Best Values at B.T.P.S - ERS Normal Values (S/W 74.215/1.00)

Index	Pred	Pre	%	Post	%	Change	
FVC	4.97	4.41	88	4.71	94	6	←
FEV1	4.03	3.80	94	3.95	97	3	
FEV1/FVC%	81	86	106	83	102	---	30 user
PEF	563	625	111	640	113	2	configurable
FEF25-75%	4.30	4.59	106	4.41	102	-4	spirometric
FIF50/FEF50%	109	135	123	127	116	---	indices

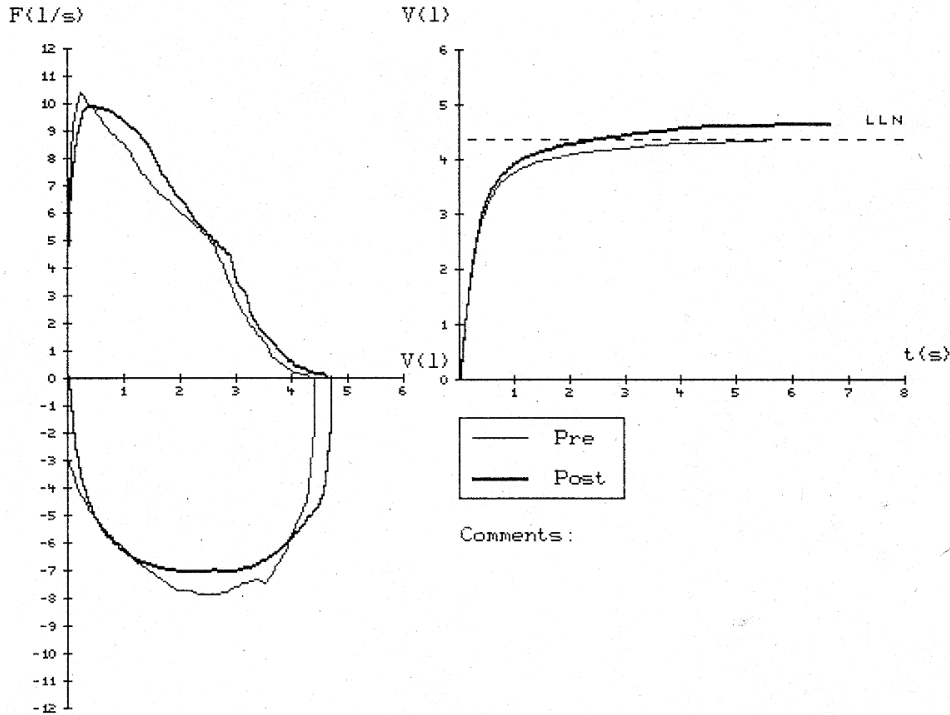

Comments:

Interpretation of Test Results:
 Normal Ventilatory Function.
 No significant Bronchodilator response.

Signature: _____

.... from **Vitalograph®**
 the spirometry people